

RESEARCH PAPER

The Antifungal Efficacy of Heat-Cured Acrylic-Based Soft Denture Liners Infused with Magnesium Oxide Nanoparticles

Zinah Salem Awfi^{1*}, Mujha Ahmed², Duha Mahdi Hussein³, Shaymaa Abdulhameed Khudair⁴, Ahmed S. Abed⁵, Anwar abdalabass Algaber⁶

¹ Department of Dental Industry Techniques, Al-Noor University College, Bartella, Iraq

² College of Medical Technology, Al-Farahidi University, Iraq

³ Department of Medical Laboratory Techniques, Al-Mustaqbal University College, 51001 Hillah, Babylon, Iraq

⁴ Advanced Biomedical Science/ Al Nisour University College, Baghdad, Iraq

⁵ Department of Prosthetic Dental Technology, Hilla University college, Babylon, Iraq

⁶ Mazaya University College, Iraq

ARTICLE INFO

Article History:

Received 04 April 2022

Accepted 20 June 2022

Published 01 July 2022

Keywords:

Antifungal activity

MgONPs

Nanoparticle

Soft liner

ABSTRACT

Candida albicans (*C. albicans*) colonization of denture soft lining materials can cause clinical issues and material deterioration. Given their antibacterial qualities, of magnesium oxide nanoparticles (MgONPs) have generated interest for usage in biomedical applications. This research intended to determine how adding MgONPs to a soft heat-cured acrylic resin denture liner influenced its water sorption, solubility, antifungal activity, and color modification. Moreover, assessing the quantity of MgO released. Soft denture liner was infused with 0.1%, 0.2%, and 0.3% of MgONPs. A total of 200 specimens have been prepped and separated into four groups based on the test that will be run. The antifungal effects of a composite material comprised of a soft liner and MgONPs were determined using a viable count of *C. albicans* in combination with a disk-diffusion method (DDM). Using atomic absorption spectroscopy (AAS), researchers could determine the amount of MgO released by synthetic saliva. The findings of the measurements of the color change, shear bond strength, solubility, and water sorption have been statistically examined. When compared to the control group, all experimental groups displayed a highly significant decline in *C. albicans* colony forming units. No inhibition zone surrounded any test specimens utilized in any of the tested groups. The incorporation of MgONPs aids in producing a soft denture liner with antifungal properties. In addition to decreasing water sorption, this addition also raised the material's opacity while having no effect on the shear bond strength.

How to cite this article

Awfi Z S., Ahmed M., Hussein D M., Khudair S A., Abed A S., Algaber A A. The Antifungal Efficacy of Heat-Cured Acrylic-Based Soft Denture Liners Infused with Magnesium Oxide Nanoparticles. J Nanostruct, 2022; 12(3):738-745. DOI: 10.22052/JNS.2022.03.026

INTRODUCTION

In order to equally disperse the stresses placed on soft tissues during function, soft liners designed for relining removable dentures and other oral and

maxillofacial prosthesis are employed [1,2]. They are polymeric materials that can be adhered to the tissue surface of a hard denture base. Denture stomatitis is a word used to characterize specific pathologic alterations in the oral mucosa of

* Corresponding Author Email: zinahsalem@alnoor.edu.iq



denture-bearing tissues below partial or complete dentures in both jaws, and somewhat often in the maxilla of denture wearers, mostly elderly people [3–5]. Wearers of full dentures have a reported prevalence of 11-67% [6]. According to reports in the literature, *Candida* species are frequently linked to denture stomatitis [7–11] (Fig. 1).

Clinical issues and material degradation may emerge from *Candida albicans* (*C. albicans*) colonization of denture soft lining materials. This tendency can be exacerbated by increased humidity and high temperature beneath the dentures, as well as by the material's surface characteristics. *C. albicans*, which is isolated from the surface of a soft denture liner, was identified as one of the etiological contributors to denture stomatitis [12]. In addition, several studies have demonstrated that *C. albicans* can penetrate soft lining materials at varying depths [13–16]. This may diminish the effectiveness of the various chemical cleaning agents available. Plaque control techniques, both mechanical and chemical, are frequently employed to prevent the development of denture stomatitis [17]. Some elderly and hospitalized patients with cognitive impairment, reduced motor dexterity, or memory loss may find it challenging to clean their dentures [18]. In addition, the use of these techniques can cause severe damage to the materials that comprise the soft lining [19]. Researchers across the globe are becoming interested in nanoparticles due of their antibacterial capabilities [20]. Due to the advent of infections that are resistant to antibiotics and the subsequent spread of infectious diseases, metal and metal oxide nanoparticles

are frequently employed as an antibacterial agent [21]. Magnesium oxide (MgO) is well-known for its antimicrobial properties against numerous bacteria, fungi, and viruses [22,23]. The nanoparticle has demonstrated some exceptional, encouraging outcomes concerning its use as an antibacterial agent due to its small size, large surface to volume ratio, and other primary unique properties [24]. The discovery of new antibacterial compounds may be facilitated by the capacity to manufacture metal and metal oxide nanoparticles of a certain size and form. Among all metal oxide nanoparticles, MgO nanoparticles have received the most attention for their antibacterial properties [25]. In this research, in order to inhibit *C. albicans*-induced microbial growth, magnesium oxide nanoparticles (MgONPs) are incorporated into an acrylic-based soft denture liner. In addition to determining the amount of MgO released, the study examined whether adding MgONPs would significantly alter the mechanical and physical properties of the soft lining material.

MATERIALS AND METHODS

In this investigation, a soft acrylic-based denture liner was used (GC Dental Industrial Corp., Tokyo, Japan). The soft liner contained 0.1%, 0.2%, and 0.3% of MgONPs. These percentages represent the weight of the powder. Their separation followed the preparation of 200 specimens into four distinct groups, each determined by the type of examination to be conducted. A To ascertain whether a chemical interaction occurs between the MgONPs and the soft liner, Fourier-transform infrared spectroscopy (FTIR) was used. Fig. 2


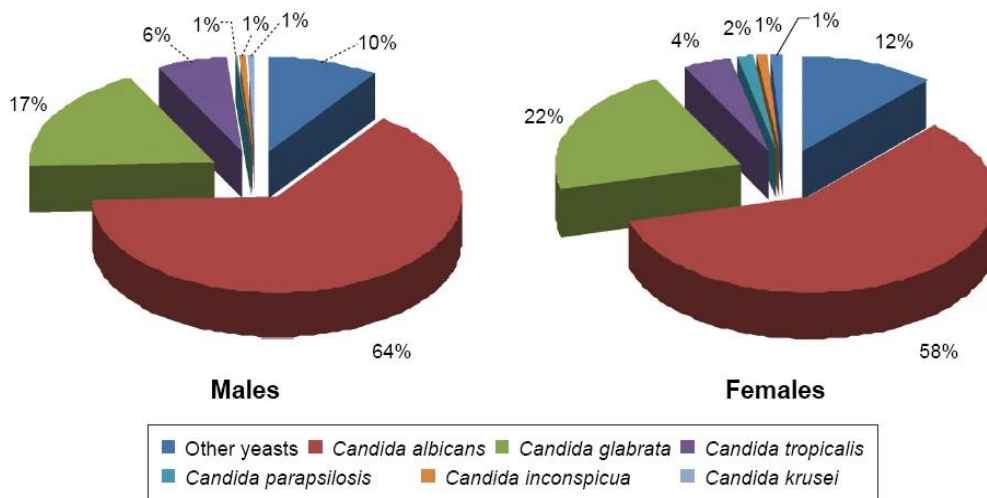


Fig. 1. The most prevalent *Candida* species found in both males and females.



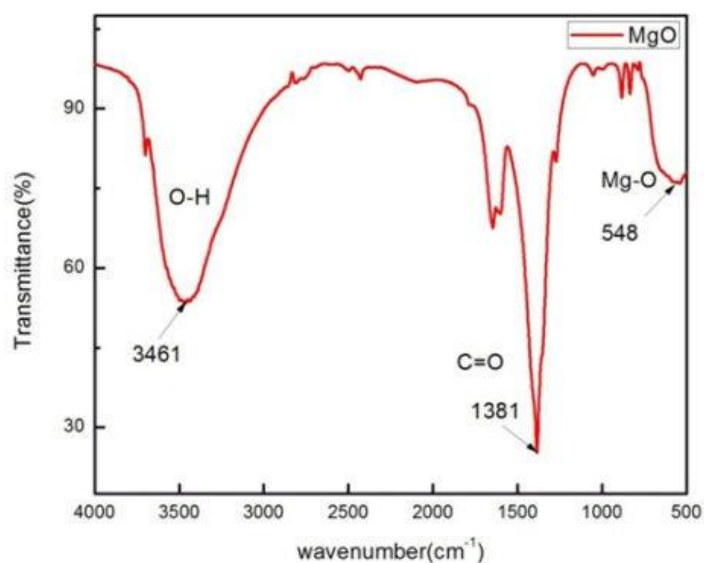

(a)

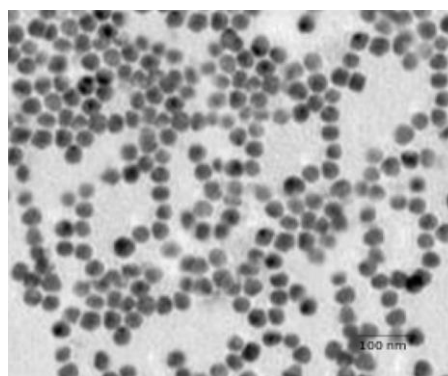
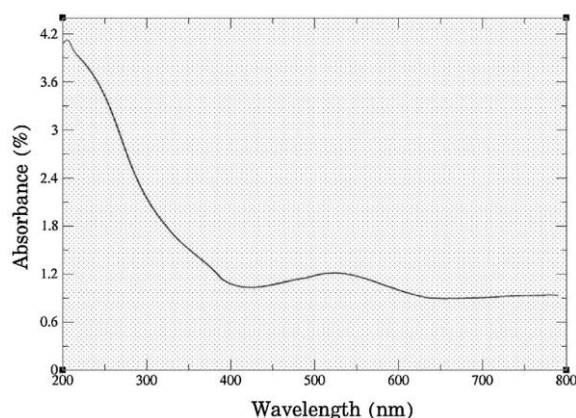


Fig. 2. Analysis results of MgONPs: (a) FTIR spectroscopy, (b) absorption spectra, and (c) TEM image.

shows the FTIR spectra, the absorption spectra and the transmission electron microscope (TEM) image of the MgONPs acquired.

A broad band at around 433-769 cm⁻¹ is assigned to the metal-oxygen bending vibration. A broad band at around 3461 cm⁻¹ is attributed to stretching frequency of H-O-H. The broad band near 1381 cm⁻¹ is due to C=O stretching frequency shows the presence of aromatic ring. Specimens of 10×10×2mm dimensions were prepared using plastic patterns to create a silicon-stone mould [26]. According to the manufacturer's specifications, each specimen was prepared, packaged, and cured. After adding the MgO NPs to the liner monomer, a probe sonication device was used for three minutes to disperse the MgO NPs and create individual nanoparticles

(Soniprep-150, MSE, Sussex, UK). The container was submerged in a cooling bath, sometimes known as an ice-water bath, to prevent excessive liquid evaporation or material degradation caused by the mixture heating up during sonication [27]. After the specimens had fully cured, a final polish was applied, and they were autoclaved to ensure sterility. By rubbing the lesional tissue with a sterile cotton swab, 20 people with denture stomatitis and oral thrush had *C. albicans* isolated from their mouths. After that, the organism was grown on Sabouraud Dextrose Agar (SDA) for 24 to 48 hours and kept at 37°C. When it forms pasty convex, smooth, creamy colonies on SDA [28], the colony morphology and gram stain were used to identify it. Additionally, a Germ Tube Test (GTT) approach was performed [29–31], and API Candida system

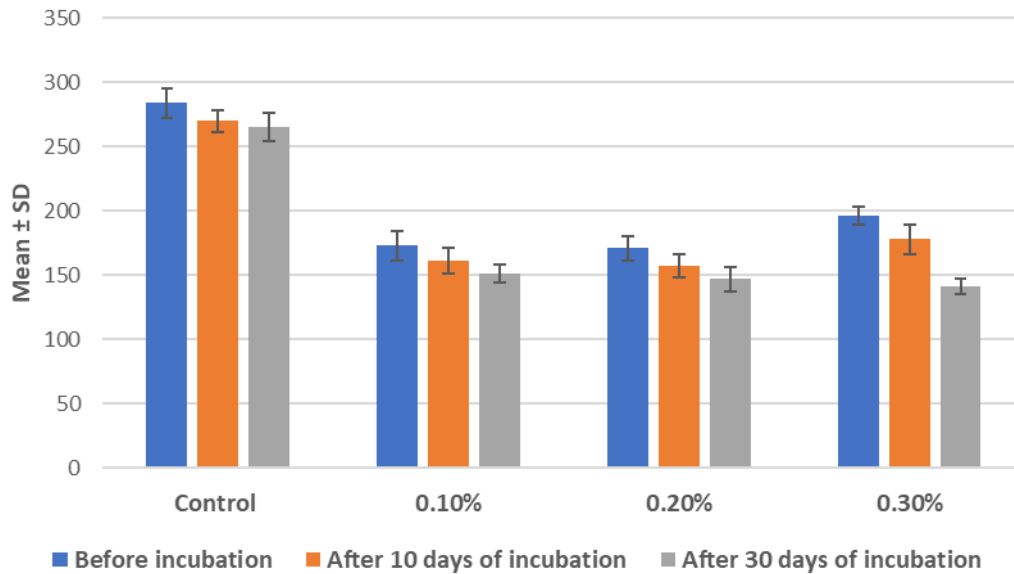


Fig. 3. Viable *C. albicans* count for all study groups and for various time periods (P<0.05).

(bioMérieux, France) was used for the biochemical method's final verification [32,33]. To evaluate the antimicrobial activity of the soft liner/MgONPs composites, *C. albicans* was diluted in 1% NaCl. A yeast suspension containing approximately 10^7 CFU/ml was prepared using the McFarland density method (0.5 McFarland standard) [34]. After placing each sample in a tube containing 10 mL of SDA broth, 100 μ L of yeast suspension was added to each tube. A final cell density of 10^5 CFU/ml was achieved. After 24 hours of incubation at 37°C,

100 μ L of each mixture were diluted tenfold by adding them to 10 mL of NaCl solution. 100 μ L of the second dilution was spread out on SDA before being incubated aerobically at 37°C for 24 hours. After storing the specimens in synthetic saliva at 37°C for 10 days and 30 days, this procedure was repeated. In this examination, specimens with a diameter of 8 mm and a thickness of 0.5 mm were utilized. The testing substrate for this experiment was Mueller-Hinton agar containing 2% glucose and 5 μ g/ml of methylene blue (prepared in

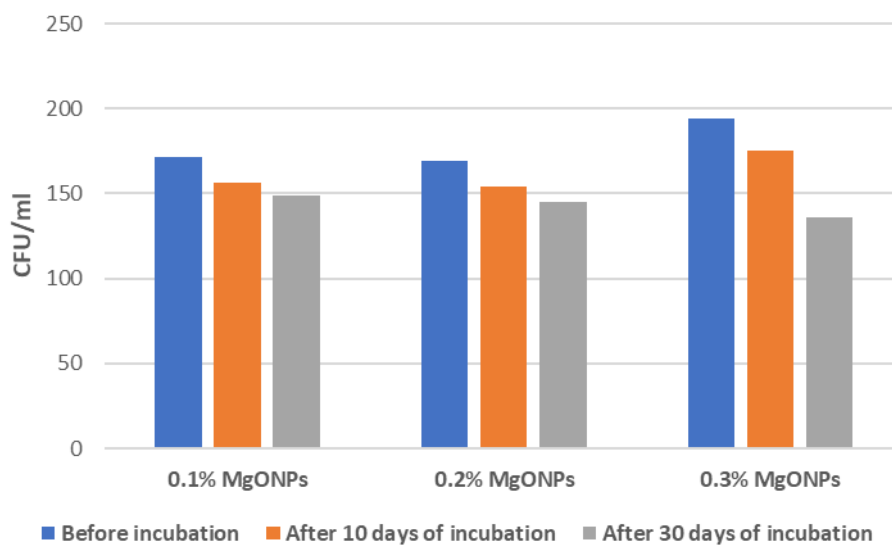


Fig. 4. Mean CFU/ml values for each experimental group at various research intervals.

accordance with the manufacturer's guidelines) [35]. The decision was made to perform a Kirby-Bauer disk diffusion susceptibility test. Five-well colonies of *C. albicans* were suspended in 0.85% sterile normal saline containing 5 mL to accomplish a turbidity of 0.5 McFarland in order to produce a yeast stock suspension. After dipping a clean swab into the inoculum suspension, the sterile swab was used to squeeze out any excess fluid. The agar plate was swabbed three times to ensure uniform growth [36]. After leaving the agar surface alone for approximately 5 min, MgO NPs-containing and MgO NPs-free soft liner disks are placed on the agar. The plates are then stored at room temperature for 120 min to permit the antimicrobial agents to diffuse throughout the agar [37]. Finally, the agar plates undergo an aerobic incubation at 37°C for 24 hours. A digital caliper is used to measure the potential inhibition zone that may form around the disks. Specimens measuring 3 mm in thickness, 10 mm in diameter and two atomic absorption spectrophotometers (AAS), with detection limits of 0.025ppm and 0.015ppb, respectively, were used to determine the amount of MgO that was released (Model: ELICO SL194) [38]. Every ten days, the volume of synthetic saliva was reconstituted to account for natural evaporation. In each period (T1=10 days; T2=30 days), the solution from each tube was collected, and the amount of MgO released was determined using AAS. For the experimental and control specimens, 0.5±0.05 mm thickness and 50±1 mm diameter metal disks were manufactured using American National Standards Institute/American Dental Association Specification No.12 compliant metal patterns. All disk-shaped specimens were dried at 37°C±2°C for 24 hours in a desiccator containing dry silica gel, cooled to room temperature for 1 hour, and then weighed using a digital electronic balance with an accuracy of 0.0001g. This cycle was repeated until a constant weight (±0.5 mg) was reached. This was taken into account as the initial weight (W1). The samples were then heated for 7 days at 37°C±2°C in distilled water. After this time, each specimen was removed from the water, wiped with a clean, dry hand towel until all visible moisture was removed, waved in the air for 15 seconds, and weighed 1 min later (W2). The specimens were then dried in a desiccator and weighed every 24 hours until they reached a constant weight (±0.5 mg). This weight reflects the quantity of the substance present (W3). The following formulas were used to determine the water sorption and solubility of each specimen:

$$\text{Sorption} = \frac{W2 - W1}{\text{surface area}} \text{ (mg/cm}^2\text{)},$$

$$\text{Solubility} = \frac{W1 - W3}{\text{surface area}} \text{ (mg/cm}^2\text{)}$$

Soft lining material was evaluated for shear bond strength to an acrylic denture base using acrylic blocks with specific dimensions 80×20×5mm and a stopper with an anticipated depth of 3 mm. Next, acrylic resin that has been heat-cured was employed (Lucitone 550, (LU)). All processes followed the manufacturer's instructions, including mixing, packaging, and curing. Following this, one acrylic block was placed on top of the other, and a space measuring 20×20×3.5mm was filled with wax. In order to create a mold for the final stage of the specimen's curing process, the entire specimen was cast in silicon material. After removing the wax, the formed space was filled with soft lining material and cured. The specimens were evaluated with the aid of an Instron Universal Testing Machine (PTC/O83/ME, INSTRON, USA). In order to determine the shear bond strength value for each test sample, the highest load necessary for failure was divided by the cross-section area (ASTM D 638-03 (2005)). Disk-shaped specimens with dimensions of 0.5±0.05 mm in thickness and 50±1 mm in diameter were prepared for use in Ultraviolet-Visible spectrophotometer (Shimadzu UV-1700) measurements of color change. This instrument measures the thickness of specimens and evaluates color change by measuring the percentage of absorbed light. A one-way ANOVA (analysis of variance) was used to compare the means in various groups. Values of P<0.05 were considered to be significant and values of P<0.01 highly significant.

RESULTS AND DISCUSSION

According to the FTIR analysis results, the material used for the soft lining had no chemical interaction with the MgO NPs. All experimental groups using different concentrations of MgO NPs (0.1%, 0.2%, and 0.3%) demonstrated a highly significant decrease in the number of *C. albicans* colony forming units relative to the control group (P<0.01). This decrease became more pronounced as the incubation time in synthetic saliva increased (Figs. 3 and 4).

ion test results did not reveal the existence of an inhibition zone around any test specimens. At no point during the incubation process did the synthetic saliva exhibit any signs of MgO release. The incorporation of MgO NPs resulted in a highly significant decrease in the mean value of water sorption (P<0.01) (Fig. 5). At the same time, only the 0.3% group exhibited a highly significant decrease in solubility (P<0.01) (Fig. 5). None of the test groups demonstrated statistically significant differences in shear bond strength (P>0.05) (Fig.

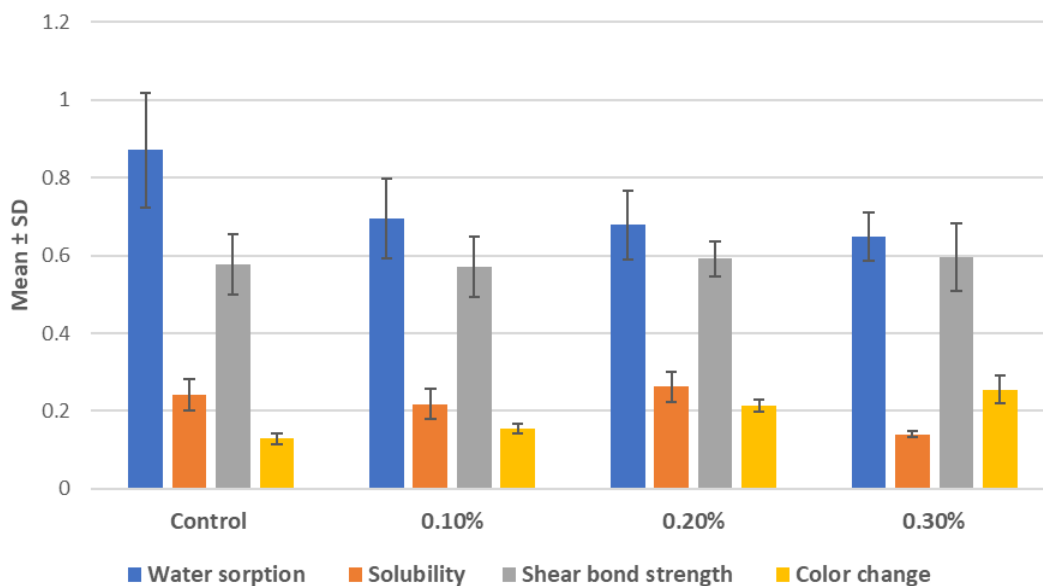


Fig. 5. Descriptive statistics of water sorption, solubility, shear bond strength and color change test results.

5). The percentage of light absorbed increased in all experimental groups and was highly significant ($P < 0.01$) (Fig. 5).

In the present study, MgO NPs were incorporated into a soft denture liner to improve the liner's antimicrobial properties against *C. albicans* yeast, one of the primary contributors to denture-induced stomatitis. After incorporating MgO NPs into the soft denture liner, the results of this study revealed a statistically highly significant reduction in *C. albicans* colony forming units per milliliter. Antimicrobial effectiveness appeared to be proportional to concentration. The length of time the composite of the tested soft liner and MgO NPs was allowed to incubate in synthetic saliva appeared to affect the composite's antifungal activity. This phenomenon may be caused by the longer duration of specimens' immersion in an aqueous environment. No MgO were discovered to be released during this process [39]. These phenomena and a reduction in water sorption may explain the substance's decreased antifungal activity and subsequent improvement (0.3%). The disk-diffusion test revealed no evidence of an inhibition zone surrounding the specimens, regardless of the percentage of MgO NPs used, even after incubating the samples in artificial saliva. This phenomenon may be explained by the absence of magnesium oxide ion release from the soft liner/MgO NPs composite, as confirmed by the results of this study. Using AAS, the researchers did not detect any MgO in the synthetic saliva at any time during incubation. This was another

finding that lent credibility to the study's findings. Previous research evaluated the release of MgO from a variety of polymeric materials [40–42]. Some of that research agreed with the present study's findings [41], while other research reached a different conclusion due to a different magnesium oxide concentration in the environment [40,42]. This could be accounted for by variations in MgO NPs incorporation techniques, polymeric material types, and polymerization processes.

CONCLUSION

In the current work, MgO NPs were added to a soft denture liner to enhance its antibacterial capabilities against the yeast *C. albicans*. The outcomes of this investigation showed a statistically highly significant decrease in *C. albicans* colony formation after adding MgO NPs to the soft denture liner.

CONFLICT OF INTEREST

The authors declare that there is no conflict of interests regarding the publication of this manuscript.

REFERENCES

1. Elawady A, Mohamed S, R N. A study to compare adhered oral flora to soft liner and conventional denture base surface in complete denture patients. *Egypt Dent J.* 2019;65(4):3777-3786.
2. Mutluay MM, Ruyter IE. Evaluation of bond strength of soft relining materials to denture base polymers. *Dent Mater.* 2007;23(11):1373-1381.

3. Olejnik M, Osmola-Mańkowska A, Ślebioda Z, Adamski Z, Dorocka-Bobkowska B. Oral mucosal lesions in psoriatic patients based on disease severity and treatment approach. *Journal of Oral Pathology & Medicine*. 2020;49(8):822-828.
4. Jhugroo C, Divakar DD, Jhugroo P, Al-Amri SAS, Alahmari AD, Vijaykumar S, et al. Characterization of oral mucosa lesions and prevalence of yeasts in diabetic patients: A comparative study. *Microb Pathog*. 2019;126:363-367.
5. Bajunaid SO, Baras BH, Weir MD, Xu HHK. Denture Acrylic Resin Material with Antibacterial and Protein-Repelling Properties for the Prevention of Denture Stomatitis. *Polymers*. 2022;14(2):230.
6. Hu L, He C, Zhao C, Chen X, Hua H, Yan Z. Characterization of oral candidiasis and the Candida species profile in patients with oral mucosal diseases. *Microb Pathog*. 2019;134:103575.
7. de Vasconcelos AA, Gonçalves LM, Del Bel Cury AA, da Silva WJ. Candida-Associated Denture Stomatitis: Clinical Relevant Aspects. *Oral Candidosis: Springer Berlin Heidelberg*; 2015. p. 53-57.
8. Cavaleiro I, Proença L, Félix S, Salema-Oom M. Prevalence of Yeast Other than Candida albicans in Denture Wearers. *Journal of Prosthodontics*. 2013;22(5):351-357.
9. Gauch LMR, Pedrosa SS, Silveira-Gomes F, Esteves RA, Marques-da-Silva SH. Isolation of Candida spp. from denture-related stomatitis in Pará, Brazil. *Braz J Microbiol*. 2018;49(1):148-151.
10. Jawale BA, Redasani R, Chaudhari L, Chopde N, Pharande A, Hiremath V. Microbial Colonization and their Relation with Potential Cofactors in Patients with Denture Stomatitis. *The Journal of Contemporary Dental Practice*. 2012;13(4):456-459.
11. Loster JE, Wieczorek A, Loster BW. Correlation between age and gender in Candida species infections of complete denture wearers: a retrospective analysis. *Clin Interv Aging*. 2016;Volume 11:1707-1714.
12. Sugio CYC, Garcia AAMN, Albach T, Moraes GS, Bonfante EA, Urban VM, et al. Candida-Associated Denture Stomatitis and Murine Models: What Is the Importance and Scientific Evidence? *Journal of Fungi*. 2020;6(2):70.
13. Takakusaki K, Fueki K, Tsutsumi C, Tsutsumi Y, Iwasaki N, Hanawa T, et al. Effect of incorporation of surface pre-reacted glass ionomer filler in tissue conditioner on the inhibition of Candida albicans adhesion. *Dent Mater J*. 2018;37(3):453-459.
14. Homsiang W, Kamonkhantikul K, Arksornnukit M, Takahashi H. Effect of zinc oxide nanoparticles incorporated into tissue conditioner on antifungal, physical, and mechanical properties. *Dent Mater J*. 2021;40(2):481-486.
15. Bertolini MM, Portela MB, Curvelo JAR, Soares RMA, Lourenço EJV, Telles DM. Resins-based denture soft lining materials modified by chlorhexidine salt incorporation: An in vitro analysis of antifungal activity, drug release and hardness. *Dent Mater*. 2014;30(8):793-798.
16. Ahmed N, Bhandari AJ, Sachdev AS, Khan F, Malhotra S, Bashir T. A clinical study of adherence of candida albicans to an improved NBR denture soft lining material. *Journal of Health and Allied Sciences NU*. 2015;05(03):036-039.
17. Skupien JA, Valentini F, Boscato N, Pereira-Cenci T. Prevention and treatment of Candida colonization on denture liners: A systematic review. *The Journal of Prosthetic Dentistry*. 2013;110(5):356-362.
18. al-Kaisy N, Saddq TH, Raouf LL. Assessment of denture hygiene habits among complete denture wearers attending Sulaimani Dental School. *Sulaimani dental journal*. 2016;3(2):69-77.
19. Martins KV, Gontijo SMDL. Tratamento da estomatite protética: revisão de literatura. *Rev Bras Odontol*. 2017;74(3):215.
20. Yin IX, Zhang J, Zhao IS, Mei ML, Li Q, Chu CH. &The Antibacterial Mechanism of Silver Nanoparticles and Its Application in Dentistry. *International Journal of Nanomedicine*. 2020;Volume 15:2555-2562.
21. Das B, Moumita S, Ghosh S, Khan MI, Indira D, Jayabalan R, et al. Biosynthesis of magnesium oxide (MgO) nanoflakes by using leaf extract of Bauhinia purpurea and evaluation of its antibacterial property against Staphylococcus aureus. *Materials Science and Engineering: C*. 2018;91:436-444.
22. Saied E, Eid A, Hassan S, Salem S, Radwan A, Halawa M, et al. The Catalytic Activity of Biosynthesized Magnesium Oxide Nanoparticles (MgO-NPs) for Inhibiting the Growth of Pathogenic Microbes, Tanning Effluent Treatment, and Chromium Ion Removal. *Catalysts*. 2021;11(7):821.
23. Fernandes M, Rb Singh K, Sarkar T, Singh P, Pratap Singh R. Recent Applications of Magnesium Oxide (MgO) Nanoparticles in various domains. *Advanced Materials Letters*. 2020;11(8):1-10.
24. Almontasser A, Parveen A, Azam A. Synthesis, Characterization and antibacterial activity of Magnesium Oxide (MgO) nanoparticles. *IOP Conference Series: Materials Science and Engineering*. 2019;577(1):012051.
25. Tang Z-X, Lv B-F. MgO nanoparticles as antibacterial agent: preparation and activity. *Brazilian Journal of Chemical Engineering*. 2014;31(3):591-601.
26. Castano V, Acosta T, Mendieta, Nunez A, Ostrosky. Cytocompatible antifungal acrylic resin containing silver nanoparticles for dentures. *International Journal of Nanomedicine*. 2012:4777.
27. Sabiha NA, Ghoneim SSM, Hessien MM. Breakdown performance of transformer oil in the presence of single-phase nanocrystalline ZnO and nano-partial substitution. *IET Science, Measurement & Technology*. 2019;13(5):737-745.
28. Kzar MY, Abood FM, Abd RS, Abas AM. ISOLATION AND IDENTIFICATION OF BACTERIAL SPECIES ASSOCIATED WITH ODONTOGENIC INFECTIONS. *Annals of Tropical Medicine and Public Health*. 2020;23(12).
29. Tamboli DP, Lee DS. Mechanistic antimicrobial approach of extracellularly synthesized silver nanoparticles against gram positive and gram negative bacteria. *J Hazard Mater*. 2013;260:878-884.
30. Semeniuc CA, Pop CR, Rotar AM. Antibacterial activity and interactions of plant essential oil combinations against Gram-positive and Gram-negative bacteria. *J Food Drug Anal*. 2017;25(2):403-408.
31. Azam A, Ahmed, Oves, Khan, Habib, Memic A. Antimicrobial activity of metal oxide nanoparticles against Gram-positive and Gram-negative bacteria: a comparative study. *International Journal of Nanomedicine*. 2012:6003.
32. KarabiÇAk N, Uludağ Altun H, Karatuna O, Hazirolan G, Aksu N, AdıLoğLu A, et al. Evaluation of Common Commercial Systems for the Identification of Yeast Isolates in Microbiology Laboratories: A Multicenter Study. *Mikrobiyol Bul*. 2015;49(2):210-220.
33. Seyfarth F, Wiegand C, Erhard M, Gräser Y, Elsner P, Hipler U-C. Identification of yeast isolated from dermatological patients by MALDI-TOF mass spectrometry. *Mycoses*. 2011;55(3):276-280.
34. Pinna A, Donadu MG, Usai D, Dore S, D'Amico-Ricci G, Boscia

- F, et al. In vitro antimicrobial activity of a new ophthalmic solution containing povidone-iodine 0.6% (IODIM). *Acta Ophthalmol (Copenh)*. 2019;98(2).
35. Fothergill AW. *Antifungal Susceptibility Testing: Clinical Laboratory and Standards Institute (CLSI) Methods. Interactions of Yeasts, Moulds, and Antifungal Agents: Humana Press; 2011. p. 65-74.*
36. In vitro Susceptibility Testing of Clinical Zygomyceteous Species isolated in Cairo, Egypt against Ten Antifungal Agents by Broth Microdilution, Disk Diffusion and E-test Methods. *Egyptian Journal of Botany*. 2016;56(1):255-267.
37. Kriplani R, Thosar N, Baliga MS, Kulkarni P, Shah N, Yeluri R. Comparative Evaluation of Antimicrobial Efficacy of Various Root Canal Filling Materials Along with Aloe vera Used in Primary Teeth: A Microbiological Study. *J Clin Pediatr Dent*. 2013;37(3):257-262.
38. Monteiro DR, Gorup LF, Takamiya AS, de Camargo ER, Filho ACR, Barbosa DB. Silver Distribution and Release from an Antimicrobial Denture Base Resin Containing Silver Colloidal Nanoparticles. *Journal of Prosthodontics*. 2011;21(1):7-15.
39. Iqbal Z, Zafar MS. Role of antifungal medicaments added to tissue conditioners: A systematic review. *Journal of Prosthodontic Research*. 2016;60(4):231-239.
40. Prabhu M, Suriyaprabha R, Rajendran V, Kulandaivelu P, Valiyaveetil S. In vivo cytotoxicity of MgO-doped nanobioactive glass particles and their anticorrosive coating on Ti-6Al-4V and SS304 implants for high load-bearing applications. *RSC Adv*. 2014;4(82):43630-43640.
41. Noori AJ, Kareem FA. The effect of magnesium oxide nanoparticles on the antibacterial and antibiofilm properties of glass-ionomer cement. *Heliyon*. 2019;5(10):e02568.
42. Nallamuthu NA, Braden M, Patel MP. Some aspects of the formulation of alginate dental impression materials—Setting characteristics and mechanical properties. *Dent Mater*. 2012;28(7):756-762.