

RESEARCH PAPER

Inhibitory Effect of ZrO₂NPs on *Candida Albicans* in Heat-Cured Acrylic-Based Soft Lining Material

Amir Fadhil Al-Tu'ma^{1*}, Zeena Dhubyan Mohammed Zaki², Randa Ahmed³, Sarah Kamil Abbood⁴, Ali Abdul Kadhim Ruhaima⁵, Zainab Jamal Hamoodah⁶, Ahmed S. Abed⁷, Irina V. Pavlova⁸

¹ Ahl Al Bayt University, College of MLT, Kerbala, Iraq

² Department of Dentistry, AlNoor University College, Bartella, Iraq

³ College of Medical Technology/ Al-Farahidi University, Iraq

⁴ Medical laboratory Techniques Department, AL-Mustaqbal University College, Iraq

⁵ AL-Nisour University College, Baghdad, Iraq

⁶ Mazaya University College, Iraq

⁷ Department of Prosthetic Dental Technology, Hilla University college, Babylon, Iraq

⁸ Belgorod State National Research University, 85, Pobedy St, Belgorod, 308015, Russian Federation

ARTICLE INFO

Article History:

Received 03 April 2022

Accepted 24 June 2022

Published 01 July 2022

Keywords:

Antifungal activity

Candida albicans

Zirconium oxide nanoparticles

ABSTRACT

The most prevalent issue that can contribute to persistent mucosal inflammation is the development of microorganisms and fungi, particularly *Candida Albicans* (*C. albicans*), on soft denture lining material. The objective of the current study is to identify the inhibitory effect of Zirconium Oxide Nanoparticles (ZrO₂NPs) on *C. albicans* in heat-cured acrylic-based soft lining material and the quantity of zirconium ions (Zr) released by the composite of soft liner and ZrO₂NPs. Soft denture liners made of acrylic were given varied ratios of ZrO₂NPs. According to the test that will be conducted, 200 samples were separated into two groups (experimental and control). The soft liner/ZrO₂NPs composite's antifungal activity was evaluated utilizing two techniques over three distinct time periods (disk-diffusion test and viable count of *C. albicans*). Atomic Absorption Spectroscopy (AAS) was used to measure the amount of Zr emitted in synthetic saliva over two separate time periods. The strength of the soft liner's shear bond to the denture base material made of acrylic was evaluated using an Instron testing equipment. Compared to the control group, there was a highly significant drop in *C. albicans* colony forming units in the experimental groups (1.5% and 2% ZrO₂NPs). Once ZrO₂NPs were added to soft liners at a rate of 2%, the shear bonding strength's mean value increased in a manner that was highly significant. As a result of this research, ZrO₂NPs could be incorporated into acrylic-based soft denture lining materials to give them antifungal qualities, which lower the risk of developing denture-induced stomatitis.

How to cite this article

Al-Tu'ma A F, Zaki Z D M., Ahmed R, Abbood S K., Ruhaima A A K., Hamoodah Z J., Abed A S., Pavlova I V. Inhibitory Effect of ZrO₂NPs on *Candida Albicans* in Heat-Cured Acrylic-Based Soft Lining Material. J Nanostruct, 2022; 12(3):771-777. DOI: 10.22052/JNS.2022.03.030

* Corresponding Author Email: amirraltoma@gmail.com



INTRODUCTION

In both full and partial removable dentures, soft denture liners are utilized to evenly disperse functional demands on the tissues supporting the appliance [1,2]. These materials are suggested for patients who have xerostomia and bruxism, immediate prostheses, thin atrophic mucosa, and bony undercuts [3,4]. Silicone elastomers or acrylic resins that have been plasticized are two types of resilient lining materials [5–7]. In order to reduce the traumatic transfer of occlusal forces to severely resorbed alveolar ridges and areas healing from surgical procedures, soft denture liners are used to produce a convenient interface across oral tissues and the denture [8–10]. However, soft liners have a porous surface due to their characteristics, composition, and structural form serving as microbial reservoirs as a result [11]. In addition to systemic diseases including respiratory infections, esophageal, oropharyngeal, chronic obstructive

pulmonary disease, pneumonia, and bacterial endocarditis, liner contamination may result in serious local problems such as discomfort, pain, delayed implant osseointegration, peri-implant infections, and implant loss. Denture users have found it to be comfortable since it acts as a pad between the oral mucosa and the base of the denture [12,13]. For instance, it's been discovered that the chemical makeup of both denture base and relining materials has an impact on a parameter called shear bond strength [14–18]. High stress concentration during function may negatively impact the health of the tissues supporting dentures. To distribute the stresses placed on soft tissues while they function, chairside hard and soft denture relining materials are utilized. Bacteria might be harbored by a weak bond, which would also encourage discoloration and lining material delamination [19]. Additionally, it is suggested that the relining denture base mechanical strength

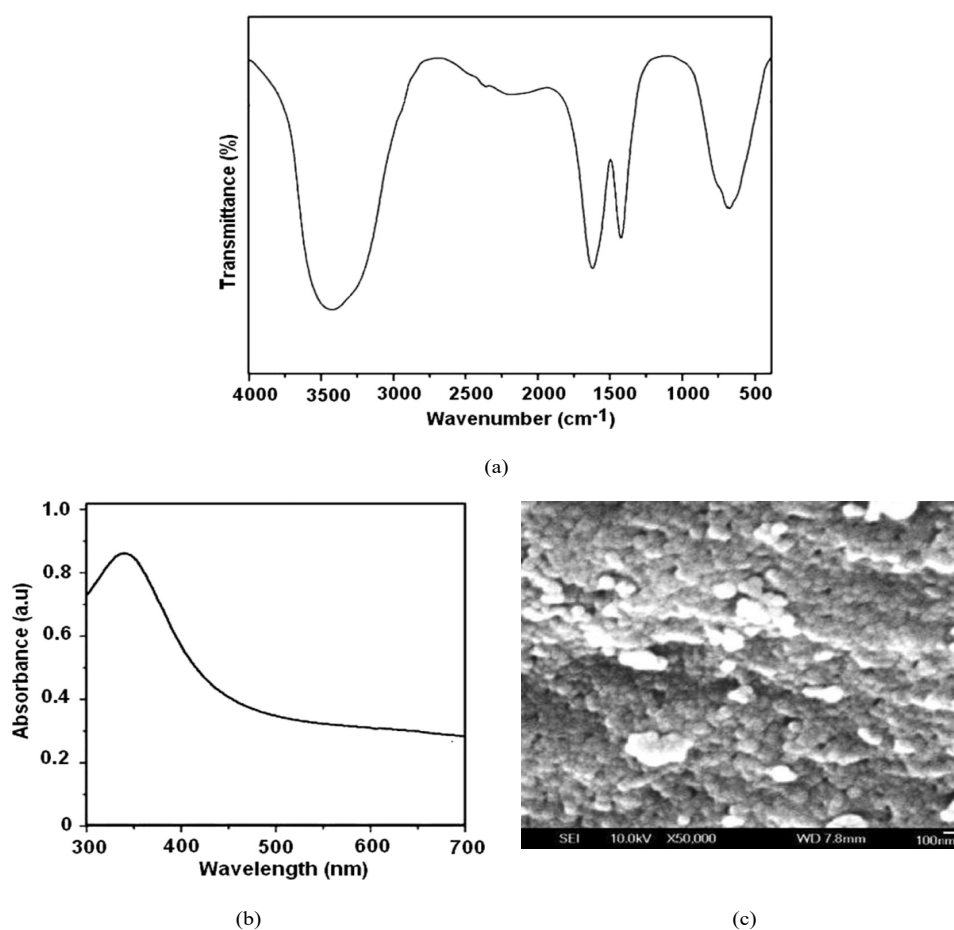


Fig. 1. Analysis results of ZrO_2 NPs: (a) FTIR spectroscopy, (b) absorption spectra, and (c) TEM image.

may be affected by the bond strength between the denture base and the resins used to make the denture relines [20,21]. *Candida Albicans* (*C. albicans*) colonization and surface roughness, that might cause denture stomatitis, are another defect [22]. Zirconium Oxide (ZrO₂) is perfect for orthopedic and dental applications due to its minimal thermal conductivity, biocompatibility, chemical stability, and superior mechanical qualities [23,24]. Invasive infections brought on by filamentous fungus have posed a significant hazard to public health during the past few years on a global scale. Human infections can be brought on by the non-filamentous fungus *Candida auris*, *Mucorales* (the most prevalent filamentous fungi), *Coccidioides*, and *Aspergillus* [25]. The innovation of new therapeutic options for the treatment of aspergillosis and infections brought on by *Candida* has employed a variety of tactics, including the incorporation of coating materials, complexes made through green chemistry, and the coupling of polymers. These human infections were chosen as additional targets for the ZrO₂ Nanoparticles (ZrO₂NPs) antifungal efficacy [25–28]. By interfering with cell activity and producing distortion in fungal hyphae, ZrO₂NPs may successfully prevent the formation of fungi [29–31].

To decrease the growth of bacteria called *C. albicans*, ZrO₂NPs have been added to an acrylic-based soft denture liner in the current research.

In order to assess Zr release, this addition was also tested to see if it had any significant effects on the material's mechanical and physical characteristics.

MATERIALS AND METHODS

In this investigation, a soft acrylic-based denture liner was used (GC Dental Industrial Corp., Tokyo, Japan). Two hundred specimens in total were prepared, and two groups (experimental and control) were created based on the test. Fig. 1 shows the transform infrared spectroscopy (FTIR) spectra, the absorption spectra and the transmission electron microscope (TEM) image of the ZrO₂NPs acquired.

Different percentages of ZrO₂NPs were applied to the soft liner (1.5% and 2% by weight). The specimens were made using plastic patterns with dimensions of 8×8×2mm [32]. According to the manufacturer's specifications, each specimen was prepared, packaged, and cured. ZrO₂NPs were introduced to the liner monomer for the experimental specimens, then dispersed for three minutes by a probe sonication equipment (Soniprep-150, MSE, Sussex, UK) to separate them into separate nanoparticles [33]. To avoid the liquid heating up in large amounts during sonication, that would lead to significant liquid evaporation or material damage, the combination was cooled down by submerging the container in a cooling bath [34]. The specimens were polished

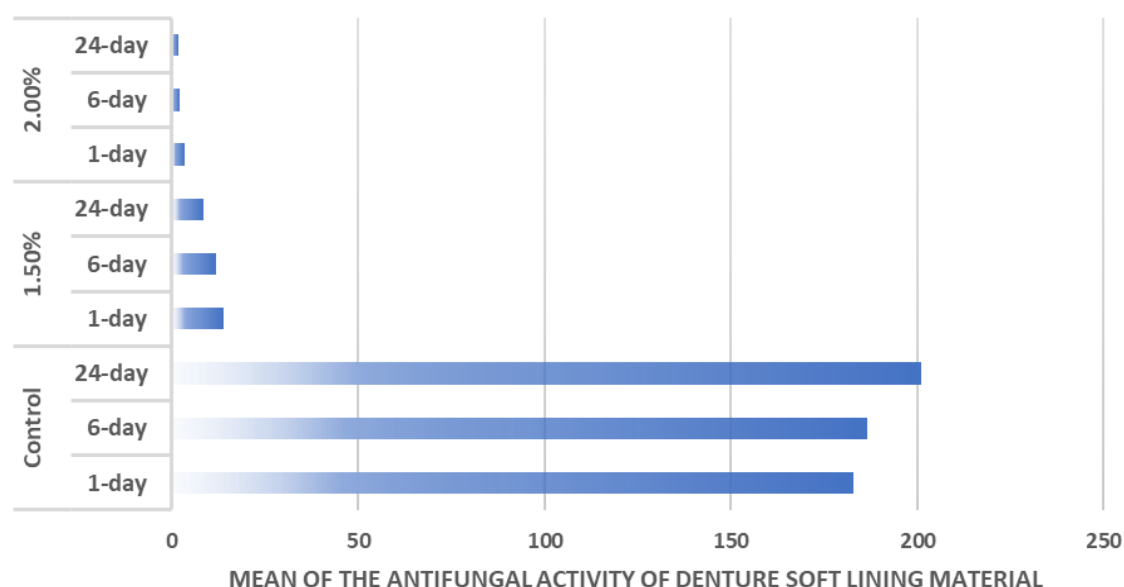


Fig. 2. Mean CFU/ml values for each experimental group over the course of the investigation at various points.

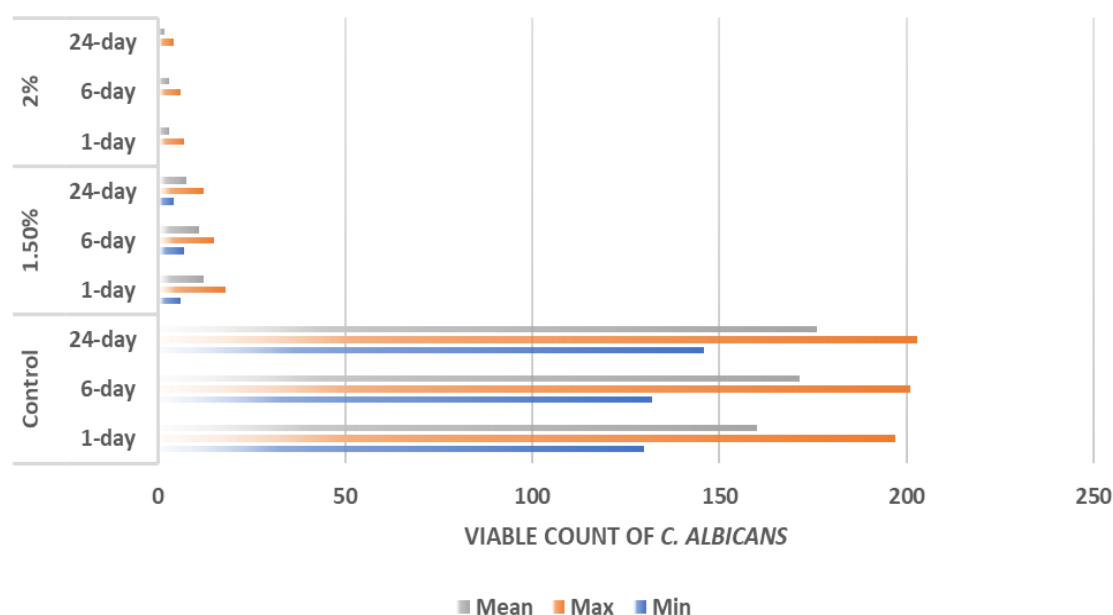


Fig. 3. For all study groups and time periods, descriptive statistics on the viable count of *C. albicans* are compared.

and made sterile by autoclaving them following complete cure. Using a sterile cotton swab, *C. albicans* was isolated from the oral cavities of 25 patients treated by the college of dentistry with symptoms of oral thrush and denture stomatitis [35]. All swab samples were initially cultured on Sabouraud Dextrose Agar (SDA), and brooded aerobically for 12 to 24 hours at 40°C, and then left at 5°C for additional analysis. When it forms pasty convex, smooth, creamy colonies on SDA, the colony morphology and gram stain were used to identify it. Additionally, a Germ Tube Test (GTT) approach was performed, and API Candida system (bioMérieux, France) was used for the biochemical method's final verification [36]. A yeast culture containing about 10⁷ CFU/ml has been created employing a McFarland densitometer and *C. albicans* to explore the antifungal efficacy of the Poly (Ethyl Methacrylate) (PEMA) matrix/ZrO₂NPs

composites (0.5 McFarland standard) [37]. Each sample was placed into a tube that held 95 µL of the yeast suspension and 10 mL of SDA. 98 CFU/mL of cells were the total cell density. After being incubated for 24 hours at 40°C, the samples were collected and washed five times in sterile deionized water in accordance with standard procedure to remove loosely connected cells. Then they were placed on SDA plates to determine the number of vital organisms. This process was repeated after storing the samples in synthetic saliva for 6 and 24 days, respectively, at 40°C. The Disk Diffusion Method (DDM) required tiny discs measuring 6mm to be carved from a rectangular metal pattern measuring approximately 30×60×0.5mm [38]. The extra fluid was squeezed out after dipping a sterile swab into the inoculum mixture. To ensure that all of the Mueller-Hinton agar supplemented with 2% glucose and methylene blue (MH-GM)'s surface

Table 1. The means of the *C. albicans* count in various groups during each incubation time were compared using a one-way ANOVA.

Incubation period	Effects	SS	Df	MS	F	P
1-day	Between groups	147987.84	2	73993.92	393.71	0.001
	Within groups	5431.59	28	201.17		
6-day	Between groups	172744.39	2	86372.19	620.74	0.001
	Within groups	3948.91	28	146.26		
24-day	Between groups	186832.87	2	93416.43	799.75	0.001
	Within groups	3338.08	28	124.33		

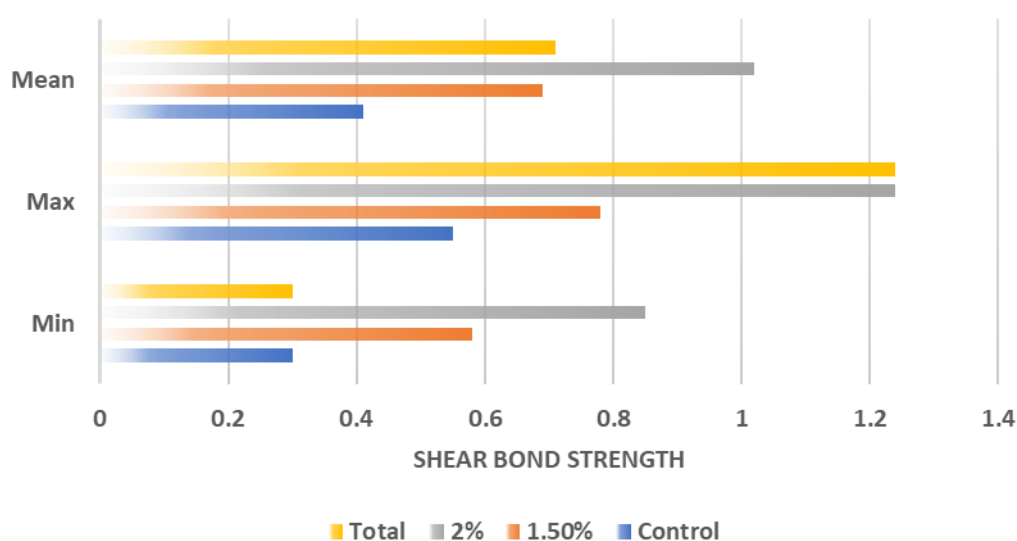


Fig. 4. Shear bond strength assessments with descriptive statistics.

Table 2. Shear bond strength test results using one-way ANOVA

Groups	SS	Df	MS	F	P
Between groups	1.77	2	0.88	113.36	0.001
Within groups	0.22	28	0.01		

area developed equally, swabbing was done in three different directions [39]. The soft-liner discs (containing and lacking ZrO₂NPs) were placed on the agar surface once it was preserved for about 5 min. The antimicrobial compounds were then allowed to diffuse over a period of 120 min while the plates remained at room temperature. For 24 hours at 40°C, these agar plates underwent aerobic incubation. A computerized electronic caliper was used to assess the inhibitory zone that might develop around the disks. Making acrylic blocks with the required measurements of 80×20×5mm and a stopper with a depth of approximately 3.5 mm was necessary in order to test the strength of shear bond of the soft lining material to the acrylic denture base [40]. Next, acrylic resin that has been heat-cured was employed (Lucitone 550, (LU)). The manufacturer's recommendations for mixing packaging and curing were followed. Afterward, one acrylic block was placed on top of the other, providing a 20×20×2.5mm wax-filled area between them. To create a mould for curing the very last specimen, the entire specimen (two wax-coated blocks) was therefore submerged in silicon material. After the wax was removed, soft lining material was placed inside the 20×20×2.5mm

chamber that had been created, and curing was then completed. In order to determine the shear bond strength value for each test sample, the highest load necessary for failure was divided by the cross-section area. To create silicone rubber molds for evaluating Zr release, a 9.5 mm in diameter and 2.5 mm in thickness plastic circular pattern was used. The proportions, mixing, and curing of experimental sample (1.5%, 2% ZrO₂NPs) were done. All samples were stored at 40°C in plastic plane tubes with 25 mL of synthetic saliva for two time points (6 and 24 days). The synthetic saliva's volume was regenerated on a regular basis to account for evaporation. Every tube's collected solution was tested for Zr dosage using Atomic Absorption Spectroscopy (AAS), and the Zr released dosage from standard solutions at different levels was counted using a linear calibration curve included into the apparatus (VarianAA-800). A one-way ANOVA (analysis of variance) was used to compare the means of the *C. albicans* count and shear bond strength test results in various groups ($P < 0.05$).

RESULTS AND DISCUSSION

According to FTIR research, ZrO₂NPs and the

soft lining material did not interact chemically. The 2% group displayed the lowest mean value (3.36 CFU/ml), which increased as the incubation duration in synthetic saliva increased (182.88 CFU/ml) (Fig. 2).

All experimental groups (1.5% and 2% ZrO₂NPs) displayed lower mean values than the control group (Fig. 3 and Table 1).

DDM demonstrated that, even after 6-days and 24-days periods of incubation in artificial saliva, there is no inhibitory zone around any of the PEMA/ZrO₂NPs discs employed in the Kirby-Bauer disk diffusion susceptibility test of any ratios of ZrO₂NPs. At any point throughout the incubation period, no Zr leakage into synthetic saliva was observed. The findings of the shear bond strength test in the current study also indicated that the 2% group had the largest mean value (1.02 N/mm²) amongst study groups, followed by the 1.5% group (0.69 N/mm²) in terms of mean value. In contrast, the control group's mean value was 0.41 N/mm² (Fig. 4 and Table 2).

By mixing ZrO₂NPs into the acrylic-based soft denture lining material, it will be possible to increase the antibacterial activity of the material against *C. albicans*, the primary culprit in denture-induced stomatitis. Due to the incorporation of ZrO₂NPs to the soft denture liner, the findings of the current investigation showed a statistically highly significant decline in CFU/ml of *Candida albicans*, demonstrating the development of a polymer with antifungal capabilities. This research supports [41] which studied the antibacterial properties of ZrO₂NPs and Zr mixed ligand complexes on bacterial strains of *S. aureus*, *E. coli*, and fungus strains of *A. niger*. The results of [42], which showed that Zr(IV) and ZrO₂ complexes with active facet play a major part in defining the activity against microorganisms, are consistent with the findings of current research. Additionally, research showed that the studied soft liner ZrO₂NPs composite's antifungal efficacy enhanced with longer incubation times in synthetic saliva.

CONCLUSION

This investigation indicated that the Zr release result was similar to the DDM, which had no inhibition zone around any specimens during Zr release. Also, no prior research has been done to show how ZrO₂NPs affect the strength of shear bond of soft lining materials. The current study's findings showed that the 2% group had

the highest mean value among the experimental groups, indicating a significant increase in the mean value of shear bond strength with increasing percentages of ZrO₂NPs added to the soft liner. Another element that enhances shear bond strength is the high flow capability of soft lining materials utilized in this research, which allows the material to adapt easily to the bonding surface and create good contact.

CONFLICT OF INTEREST

The authors declare that there is no conflict of interests regarding the publication of this manuscript.

REFERENCES

1. Hussein FA. Advances in Soft Denture Liners: An Update. *The Journal of Contemporary Dental Practice*. 2015;16(4):314-318.
2. Chladek G, Żmudzki J, Kasperski J. Long-Term Soft Denture Lining Materials. *Materials*. 2014;7(8):5816-5842.
3. Pahuja R, Kaura S, Roy N. Comparative evaluation of physical properties of commercially available silicone-based soft denture liners and acrylic-based soft denture liners. *Indian Journal of Dental Sciences*. 2020;12(1):56.
4. Faccio DR, Pereira-Cenci T, Cenci MS, Demarco FF, Moraes RR, Boscatto N. In vivo biofilm formation on a soft denture liner in elderly patients with controlled diabetes. *Gerodontology*. 2010;29(2):e143-e146.
5. Travaglini EA, Gibbons P, Craig RG. Resilient liners for dentures. *The Journal of Prosthetic Dentistry*. 1960;10(4):664-672.
6. Nowakowska-Toporowska A, Malecka K, Raszewski Z, Wieckiewicz W. Changes in hardness of addition-polymerizing silicone-resilient denture liners after storage in artificial saliva. *The Journal of Prosthetic Dentistry*. 2019;121(2):317-321.
7. Mohad A, Fatalla AA. The Effectiveness of Aluminum Potassium Sulfate Micro-Particles Addition into Soft Denture Lining Material on Tensile strength and Peel bond Strength of Soft Denture Lining Material. *Journal of Baghdad College of Dentistry*. 2019;31(4).
8. Żmudzki J, Chladek G, Malara P. Use of finite element analysis for the assessment of biomechanical factors related to pain sensation beneath complete dentures during mastication. *The Journal of Prosthetic Dentistry*. 2018;120(6):934-941.
9. Ibraheem EM, ElGabry HS. Effect of mandibular complete dentures relining on occlusal force distribution using T-scan system. *Bulletin of the National Research Centre*. 2021;45(1).
10. Białożyty-Bujak E, Wysztyńska M, Chladek G, Czelakowska A, Gala A, Orczykowska M, et al. Analysis of the Hardness of Soft Relining Materials for Removable Dentures. *International Journal of Environmental Research and Public Health*. 2021;18(18):9491.
11. Silicone versus acrylic resilient long term soft liners; a cross-over clinical study. *Current Science International*. 2020.
12. Saeed F, Muhammad N, Khan AS, Sharif F, Rahim A, Ahmad P, et al. Prosthodontics dental materials: From conventional to unconventional. *Materials Science and Engineering: C*. 2020;106:110167.
13. Onuma H, Inokoshi M, Hirayama D, Inoue M, Minakuchi S.

- Stress distribution analysis of oral mucosa under soft denture liners using smoothed particle hydrodynamics method. *J Mech Behav Biomed Mater*. 2021;117:104390.
14. Wemken G, Burkhardt F, Spies BC, Kleinvogel L, Adali U, Sterzenbach G, et al. Bond strength of conventional, subtractive, and additive manufactured denture bases to soft and hard relining materials. *Dent Mater*. 2021;37(5):928-938.
 15. Taghva M, Enteghad S, Jamali A, Mohaghegh M. Comparison of shear bond strength of CAD/CAM and conventional heat-polymerized acrylic resin denture bases to auto-polymerized and heat-polymerized acrylic resins after aging. *Journal of Clinical and Experimental Dentistry*. 2022:e72-e78.
 16. Özdemir H, Özdoğan A. Bond Strength of Resilient Lining Materials to Denture Base Resin: A Systematic Review and Meta-Analysis. *Journal of Prosthodontics*. 2018;27(9):828-841.
 17. Arun Kumar P, Iniyan K, Balasubramaniam R, Viswanathan M, Hines PJ, Monnica V. The effect of surface treatments on the shear bond strength of acrylic resin denture base with different repair acrylic resin: An in vitro study. *Journal of Pharmacy And Bioallied Sciences*. 2019;11(6):380.
 18. Hamedirad F, Alikhasi M, Hasanzade M. The Effect of Sandblasting on Bond Strength of Soft Liners to Denture Base Resins: A Systematic Review and Meta-Analysis of In Vitro Studies. *International Journal of Dentistry*. 2021;2021:1-17.
 19. Jagadeesh K, Kumar GV. A Comparative Evaluation of Shear Bond Strength between Silicone Soft Liners and Processed Denture Base Resin Conditioned by a Surface Treatment. *CODS Journal of Dentistry*. 2020;11(1):2-6.
 20. Cho S-Y, Song Y-G. A comparison study on shear bond strength of 3D printed resin and conventional heat-cured denture base resin to denture relining materials. *Journal of Dental Rehabilitation and Applied Science*. 2021;37(4):232-243.
 21. Hamanaka I, Shimizu H, Takahashi Y. Bond strength of a chairside autopolymerizing relining resin to injection-molded thermoplastic denture base resins. *Journal of Prosthodontic Research*. 2017;61(1):67-72.
 22. Kang S-H, Lee H-J, Hong S-H, Kim K-H, Kwon T-Y. Influence of surface characteristics on the adhesion of *Candida albicans* to various denture lining materials. *Acta Odontol Scand*. 2012;71(1):241-248.
 23. Chopra D, Jayasree A, Guo T, Gulati K, Ivanovski S. Advancing dental implants: Bioactive and therapeutic modifications of zirconia. *Bioactive Materials*. 2022;13:161-178.
 24. Ahmed A, Ali M. The Influence of Titanium Dioxide Nanoparticles Incorporation into Soft Denture Lining Material on *Candida albicans* Adherence and Some Mechanical and Physical Properties. *Journal of Pure and Applied Microbiology*. 2018;12(2):783-791.
 25. León-Buitimea A, Garza-Cervantes JA, Gallegos-Alvarado DY, Osorio-Concepción M, Morones-Ramírez JR. Nanomaterial-Based Antifungal Therapies to Combat Fungal Diseases Aspergillosis, Coccidioidomycosis, Mucormycosis, and Candidiasis. *Pathogens*. 2021;10(10):1303.
 26. Gowri S, Rajiv Gandhi R, Sundarajan M. Structural, Optical, Antibacterial and Antifungal Properties of Zirconia Nanoparticles by Biobased Protocol. *Journal of Materials Science & Technology*. 2014;30(8):782-790.
 27. Pholnak C, Lertworapreecha M, Sirisathitkul C, Suwanboon S. Antibacterial and physical properties of ZnO with pH-sensitive morphology. *J Exp Nanosci*. 2016;11(17):1320-1330.
 28. Karamian R, Kamalnejade J. Green synthesis of silver nanoparticles using aqueous seed extract of *Cuminum* *cuminum* L. and evaluation of their biological activities. *Journal of ilam university of medical sciences*. 2019;26(5):128-141.
 29. Sonawane H, Shelke D, Chambhare M, Dixit N, Math S, Sen S, et al. Fungi-derived agriculturally important nanoparticles and their application in crop stress management – Prospects and environmental risks. *Environ Res*. 2022;212:113543.
 30. Ejileugh C, Ezealisiji KM, Ezejiofor AN, Orisakwe OE. Microbiologically Influenced Corrosion: Uncovering Mechanisms and Discovering Inhibitor—Metal and Metal Oxide Nanoparticles as Promising Biocorrosion Inhibitors. *Journal of Bio- and Tribo-Corrosion*. 2021;7(3).
 31. Ahmad N, Jafri Z, Khan ZH. Evaluation of nanomaterials to prevent oral Candidiasis in PMMA based denture wearing patients. A systematic analysis. *Journal of Oral Biology and Craniofacial Research*. 2020;10(2):189-193.
 32. Castano V, Acosta T, Mendieta, Nunez A, Ostrosky. Cytocompatible antifungal acrylic resin containing silver nanoparticles for dentures. *International Journal of Nanomedicine*. 2012:4777.
 33. Ashour Ahmed M, El-Shennawy M, Althomali Y, Omar AA. Effect of Titanium Dioxide Nano Particles Incorporation on Mechanical and Physical Properties on Two Different Types of Acrylic Resin Denture Base. *World Journal of Nano Science and Engineering*. 2016;06(03):111-119.
 34. Sabiha NA, Ghoneim SSM, Hessian MM. Breakdown performance of transformer oil in the presence of single-phase nanocrystalline ZnO and nano-partial substitution. *IET Science, Measurement & Technology*. 2019;13(5):737-745.
 35. Oral Microbiology and Immunology, Third Edition. American Society of Microbiology; 2019.
 36. Crossman M, Willem A, Finucane P, Jennings A, Lovell BC. A multiple covariance approach for cell detection of Gram-stained smears images. 2015 IEEE International Conference on Acoustics, Speech and Signal Processing (ICASSP); 2015/04: IEEE; 2015.
 37. Monteiro DR, Gorup LF, Takamiya AS, de Camargo ER, Filho ACR, Barbosa DB. Silver Distribution and Release from an Antimicrobial Denture Base Resin Containing Silver Colloidal Nanoparticles. *Journal of Prosthodontics*. 2011;21(1):7-15.
 38. In vitro Susceptibility Testing of Clinical Zygomyceteous Species isolated in Cairo, Egypt against Ten Antifungal Agents by Broth Microdilution, Disk Diffusion and E-test Methods. *Egyptian Journal of Botany*. 2016;56(1):255-267.
 39. Pasquetti M, Chiavassa E, Tizzani P, Danesi P, Peano A. Agar Diffusion Procedures for Susceptibility Testing of *Malassezia pachydermatis*: Evaluation of Mueller-Hinton Agar Plus 2 % Glucose and 0.5 µg/ml Methylene Blue as the Test Medium. *Mycopathologia*. 2015;180(3-4):153-158.
 40. García-Domínguez A, Claver J, Camacho AM, Sebastián MA. Considerations on the Applicability of Test Methods for Mechanical Characterization of Materials Manufactured by FDM. *Materials*. 2019;13(1):28.
 41. Mukunda DA. Efficacy of *Psidium guajava* leaf extract on *Streptococcus mutans* and *Enterococcus faecalis* – an in vitro study. *Journal of Medical Science And clinical Research*. 2019;7(5).
 42. Fathima JB, Pugazhendhi A, Venis R. Synthesis and characterization of ZrO₂ nanoparticles-antimicrobial activity and their prospective role in dental care. *Microb Pathog*. 2017;110:245-251.